Alliance Analytical Laboratories, Inc.

179 West Randall Street Coopersville, MI 49404 Phone: (616) 837-7670

Fax: (616) 837-7701





Test methods marked with ^ are accredited under the laboratory's ISO/IEC 17025:2017 accreditation issued by ANSI National Accreditation Board. Refer to certificate and scope of accreditation AT-2044

TEST RESULTS REPORT


SAMPLE DESCRIPTION Kratom Leaf Powder Lot X (1-10)

SAMPLE DATE

DATE RECEIVED 10/26/2024

REFERENCE NUMBER 2029941: 2460217 Customer PO

TEMPERATURE AT RECEIVING

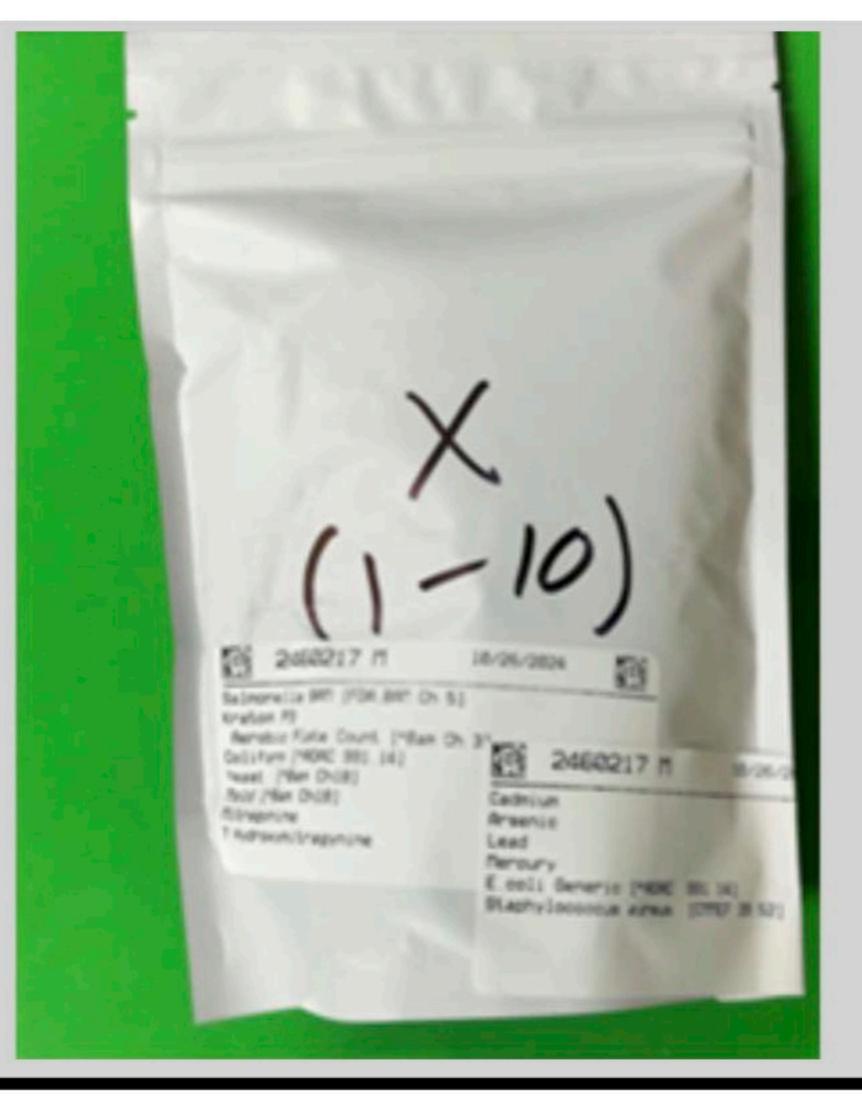

Test Requested	Test Method		Results	Ref Number	Start Date
Kratom P3					
7 Hydroxymitragynine			<0.01 %	20136:76	11/5 4:03 PM
	Analyst: 55				
Mitragynine			1.65 %	20136:76	11/5 4:03 PM
	Analyst: 55				
Aerobic Plate Count	^Bam Ch 3 Analyst: 57	Log: 2.6	400 cfu/g		10/28 3:16 PM
Coliform	^AOAC 991.14 Analyst: 57	Log: <2.0	<100 cfu/g		10/28 3:16 PM
Mold	^Bam Ch18 Analyst: 57	Log: <2.0	<100 cfu/g		10/28 3:16 PM
Staphylococcus aureus	CMMEF 39.52 Analyst: 57		<3 mpn/g		10/28 3:16 PM
Yeast	^Bam Ch18 Analyst: 57	Log: <2.0	<100 cfu/g		10/28 3:16 PM
E.coli Generic	^AOAC 991.14 Analyst: 57	Log: <2.0	<100 cfu/g		10/28 3:16 PM
Arsenic			< 0.5 mg/kg	20138:16	10/29 6:32 AM
	Analyst: 45				
Cadmium			< 0.5 mg/kg	20138:16	10/29 6:32 AM
	Analyst: 45				

It is the customer's responsibility to evaluate the compliance of these results to any regulatory requirement. Test results apply to the sample as received.

THIS DOCUMENT CONTAINS TRADE SECRET/CONFIDENTIAL INFORMATION PURSUANT TO 5 U.S.C.(b)(4)

This report must not be reproduced, except in full, without written approval of the laboratory.

Reviewed and Approved by:

Date: 11/7/2024

Audrey Monroe - Laboratory Director

Page 1 of 2

11/7/2024

Date: